

<b>Bulletin Number:</b> MI_IB_0078	<b>Distribution Date:</b> 02/7/2024	<b>Effective Date:</b> Ongoing
<b>Contact Point:</b> Metrc® Support	<b>Subject:</b> New Lab Test Batch	
<b>Reason:</b> Metrc and the CRA are providing an update on the addition of the Vape Surveillance Lab Test Batch.		


Greetings,

Metrc and the CRA are pleased to provide an update and guidance on an additional lab test batch. This bulletin will include the update on a new Vape Surveillance lab test batch feature that has been added as an option for CRA-requested audits conducted by licensed SCFs.

Please see the following pages for details on these changes:

## Vape Surveillance Lab Test Batch

Now when creating test sample packages, there will be a new “Vape Surveillance” lab test batch as an option for selection as a required lab test batch for the sample package. Vape Surveillance is to be used when the CRA instructs a licensee to create a test sample of product – see **Figure 1**.

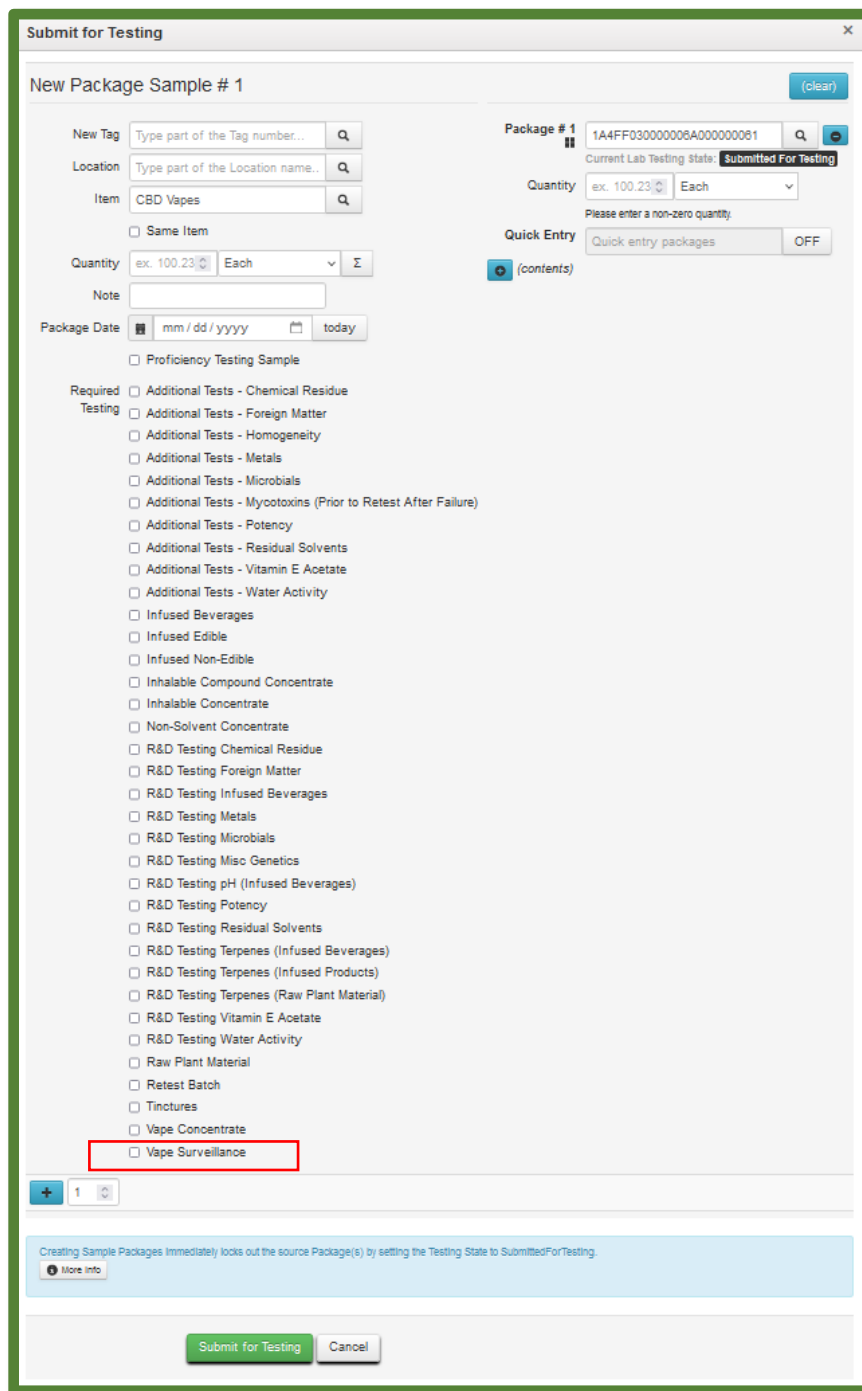

**Figure 1: Vape Surveillance Lab Test Batch Option**